


FIG. 1





1 2 3 4 5 6


FIG. 2



1 2 3 4 5 6

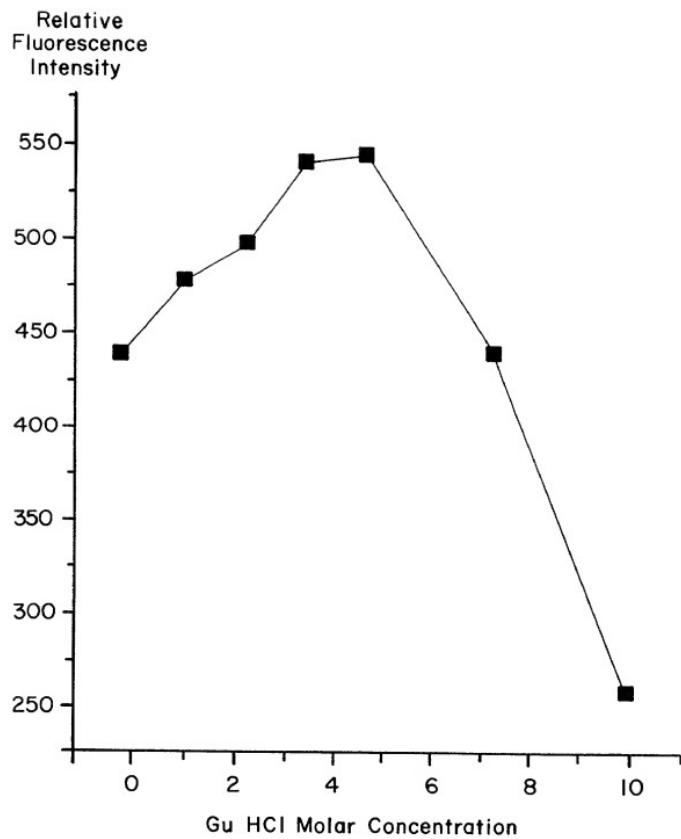**FIG. 3**

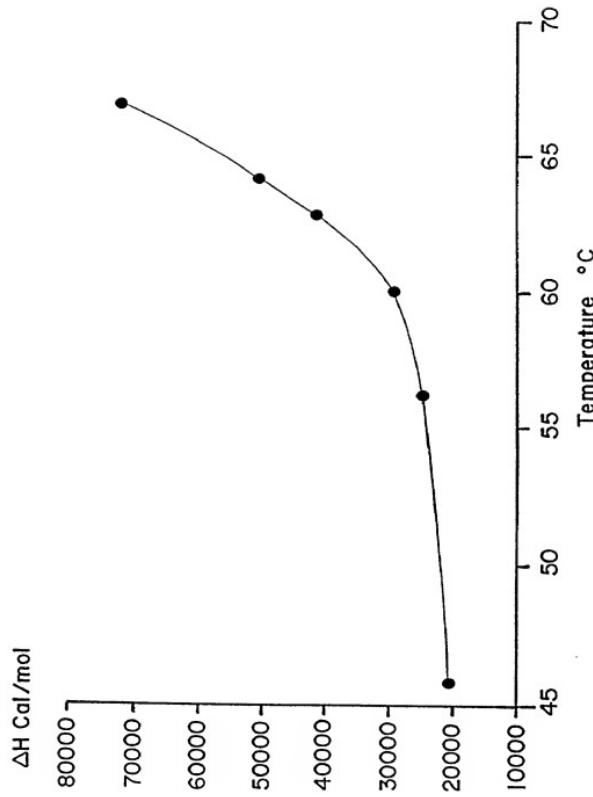**FIG. 4**

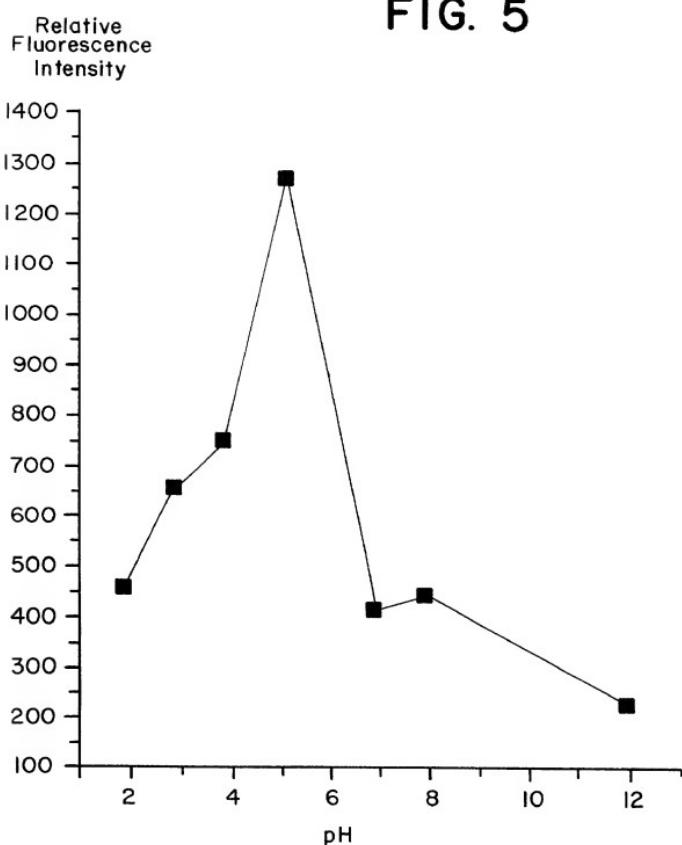**FIG. 5**

5/30

FIG. 6

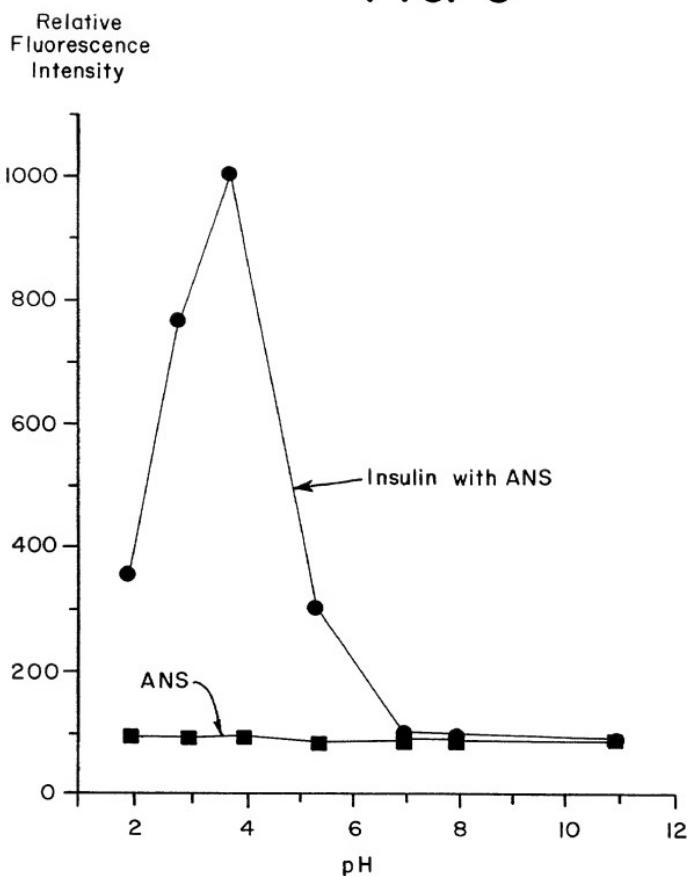


FIG. 7A

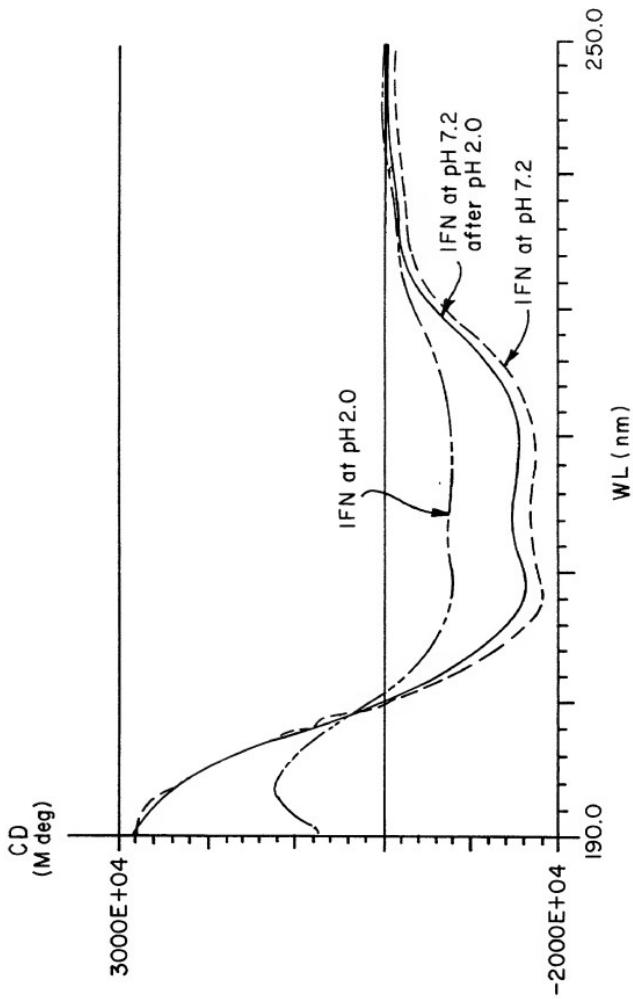


FIG. 7B


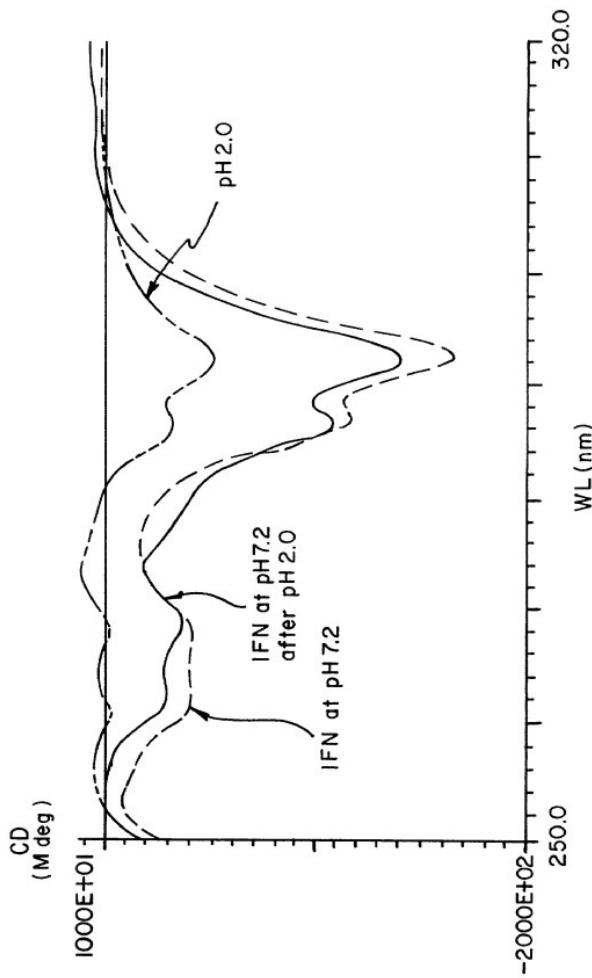


FIG. 8





**FIG. 9**

FIG. 10

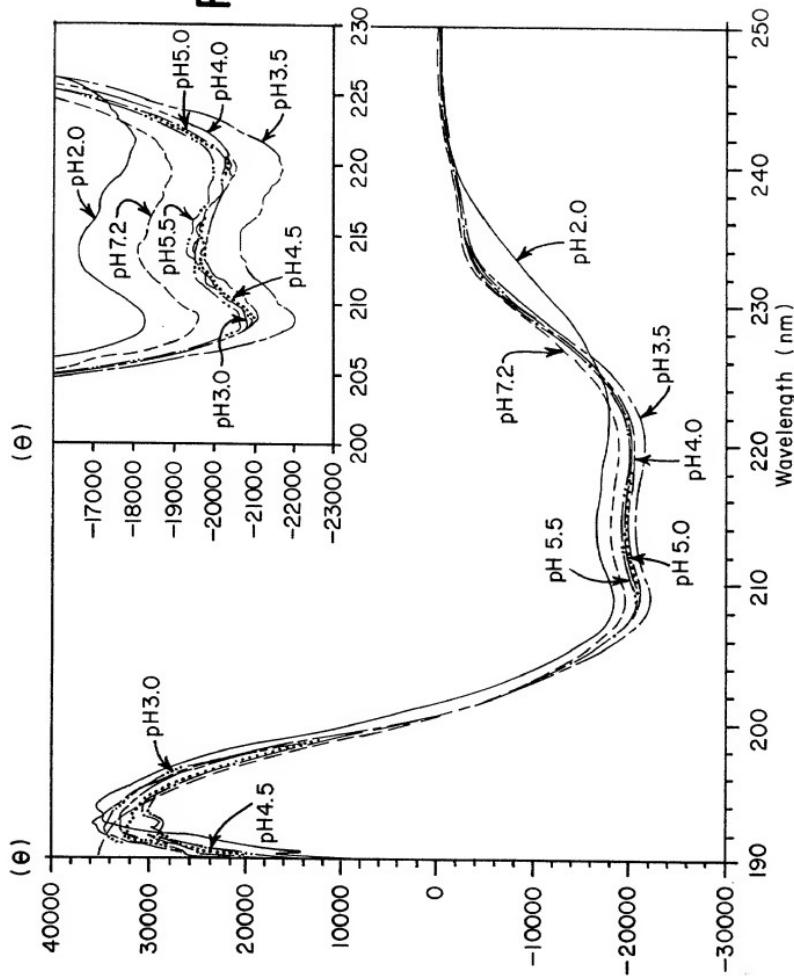

11/30

Cp  
cal/K-mol  
20000 BASELINE - BUFFER;  
SCAN RATE;  
CONC. NORM;

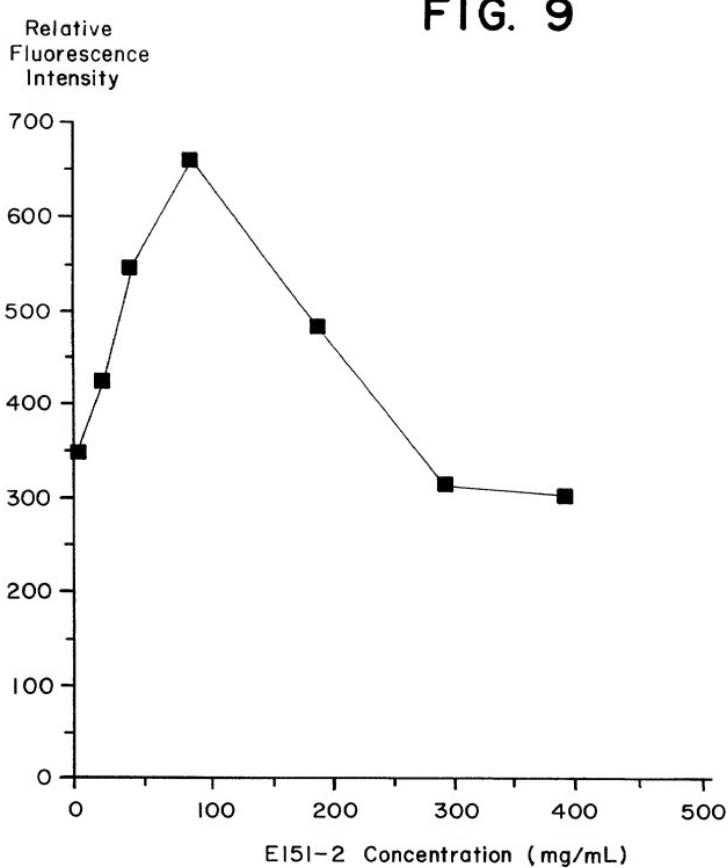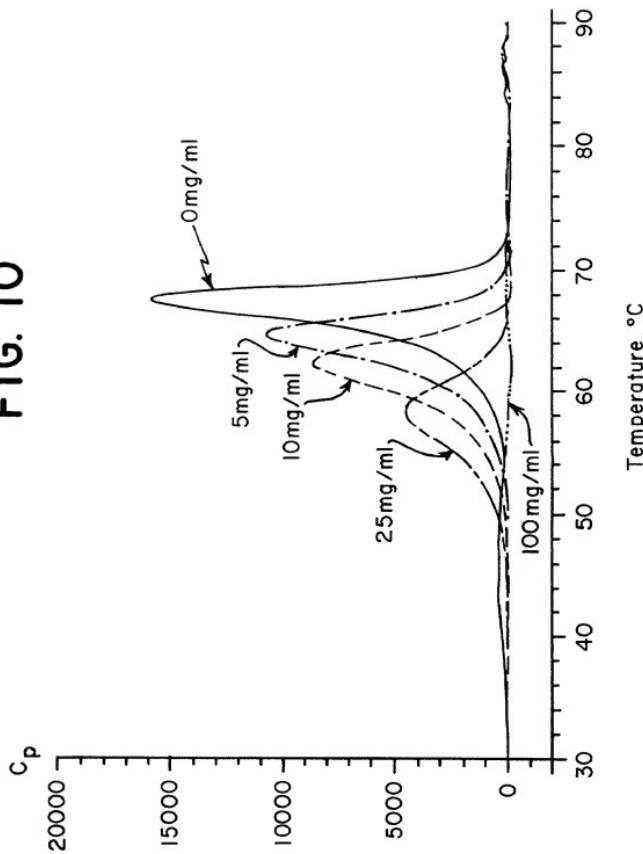